RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Dräger medical
A Dräger and Siemens Company

Field Service Procedure

Part Number: SP00288
Rev: A
Date: 19 December 2003
© 2003 Draeger Medical, Inc.

AGS Scavenger Installation

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

AGS Scavenger Installation

INSTALLATION PROCEDURE

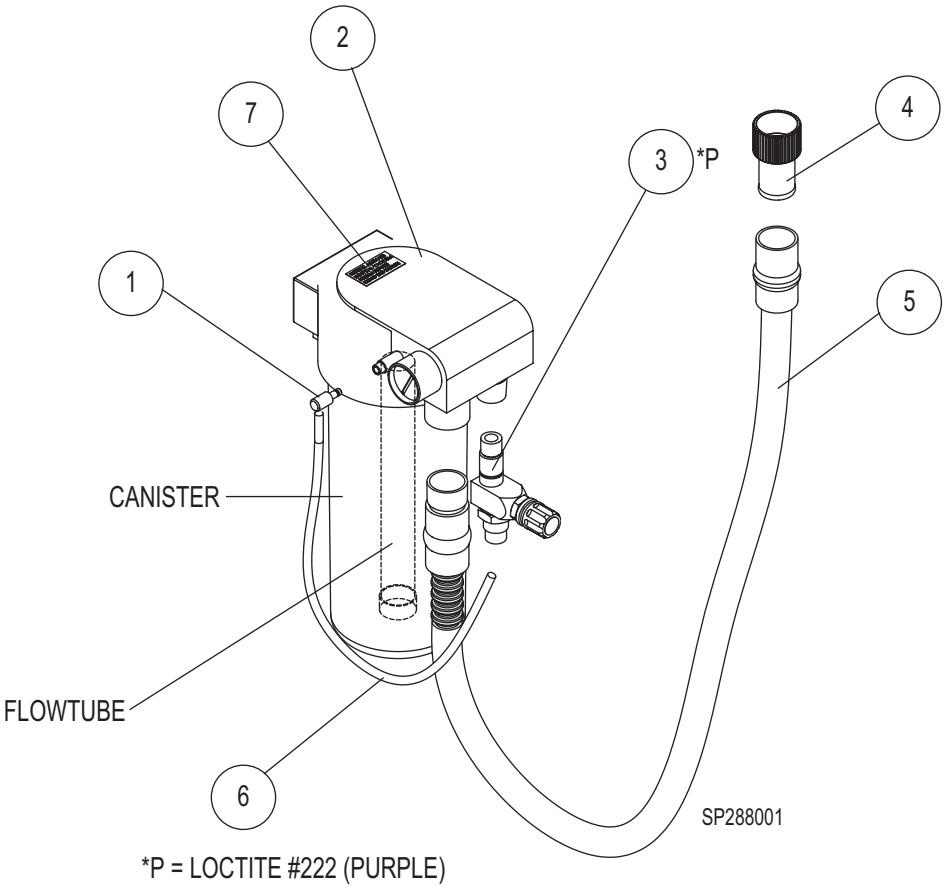

FIGURE 1. AGS Scavenger Installation

1. Remove the canister and flow tube from the bottom of the scavenger housing (2).
2. If equipped, apply a small amount of Loctite #222 to the threads of the adjustment valve (3) and screw the valve into the small port of the scavenger (2) until the threads bottom, then back off the valve to the position as shown in Figure 1, but not more than one full turn from bottom position.
3. Position the flow tube so the graduations face toward the front of the machine when the scavenger is mounted.
4. Reinstall the canister.
5. Insert the metal end of the scavenger hose (5) into the large port on the scavenger (2) and twist to secure the hose.

INSTALLATION PROCEDURE (continued)

6. Push the 30 mm adapter (4) onto the other end of the scavenger hose (5).
7. Connect the 30 mm adapter to the scavenger port on the underside of the breathing system and twist to secure.
8. If applicable, cut the smaller diameter hose (6) to the desired length for connecting an agent monitor exhaust to the scavenger.
9. Slide the hose onto the barb of the quick disconnect fitting (1) and connect the fitting to the scavenger.
10. Apply label (7) in the approximate position shown in Figure 1.

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Dräger medical

A Dräger and Siemens Company

DrägerService is a division of
Draeger Medical, Inc.
3122 Commerce Drive
Telford, PA 18969
Tel: (215) 721-5402
(800) 543-5047
Fax:(215) 721-5784
Web: www.draegermedical.com
Printed in the U.S.A.